

**Specifications of Dental Chair for Dental College RIMS Imphal.**

Dental chair and unit electrically operated with the following minimum basic items.

(A)

- (i) Air Rotor points
- (ii) 3 way syringe points
- (iii) Airmotor / micromotor
- (iv) Suction high &/or medium and low
- (v) X-Ray viewer (LED)
- (vi) Light: - Max intensity not less than 20000 lux, and
- (vii) Other accessories.

(B) Compressor oil free, low noise :- 1HP, 2HP, 3HP approx capacity separately

(C) (i) Hand pieces for Air rotor - different varieties with specification and model.

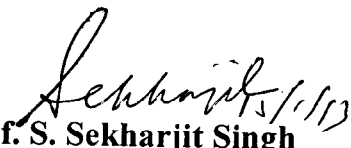
(ii) Hand pieces for Airmotor/ Micromotor

(D) Optional accessories such as

- (i) Scaler
- (ii) Light cure
- (iii) Burrs
- (iv) Ultrasonic cleaner &
- (v) Other accessories

may be quoted separately with specifications and model.

- Literature
  - Catalogue
  - Client / installation base
- } To be enclosed

  
**Prof. S. Sekharjit Singh**  
Director,  
Regional Institute of Medical Sciences,  
Imphal