

Corrigendum for 16 Slice CT Scan machine:

The following changes are made from previous specifications and terms & conditions.

- a). The supply and installation of equipments for 16 slices CT scan machine is 120 days from date of issue of supply order.
- b). The supply and installation of 16 Slices CT machine will be on Turnkey basis. The following items should be included on Turnkey basis.
 - i).Air Conditioner for whole system
 - ii).Lead Glass Window
 - iii).Lead Door
 - iv).LED view Box
 - v).Earthling wire for whole system
 - vi).Dehumidifier (2 nos.) & Electronic pest control 3 nos.

Sl.No. of the Technical Spesification:

1. Scan Time:

Scan time for one gantry of complete 360 degree rotation should be 1 sec or less.

4. Detectors:

Data acquisition system capable of acquiring of 16 slice or more per 360 degree rotation with 16 or more rows of detector. Total coverage of the detectors must be 11 mm or more.

8. X-ray Generator

High frequency time ; Power output : 24 KW or higher voltage selection: 70-130 or wider.

mA Range: 180 mA or more

20. CT Flouroscopy for Biopsy :

To be deleted from the tender specification.

21. Accessories:


Single head pressure injector with 100 syringe should be supplied.


Full system UPS from reputed manufacturer having at least **30 minutes** backup with appropriate KVA to be supplied.


22. Standard and Safety:

Should be US FDA / CE approved, AERB approved.

Sl.no. 48 of term and conditions i.e "Downtime penalty clause during warranty and CAMC period", --- Purchase Section may take the decision.


22.8.19


23.8.19


23/8/19

Corrigendum for 16 Slice CT Scan machine:

The following changes are made from previous specifications and terms & conditions.

- a). The supply and installation of equipments for 16 slices CT scan machine is 120 days from date of issue of supply order.
- b). The supply and installation of 16 Slices CT machine will be on Turnkey basis. The following items should be included on Turnkey basis.
 - i).Air Conditioner for whole system
 - ii).Lead Glass Window
 - iii).Lead Door
 - iv).LED view Box
 - v).Earthing wire for whole system
 - vi).Dehumidifier (2 nos.) & Electronic pest control 3 nos.

Sl.No. of the Technical Spesification:

1. Scan Time:

Scan time for one gantry of complete 360 degree rotation should be 1 sec or less.

4. Detectors:

Data acquisition system capable of acquiring of 16 slice or more per 360 degree rotation with 16 or more rows of detector. Total coverage of the detectors must be 11 mm or more.

8. X-ray Generator

High frequency time ; Power output : 24 KW or higher voltage selection: 70-130 or wider.

mA Range: 180 mA or more

20. CT Flouroscopy for Biopsy :

To be deleted from the tender specification.

21. Accessories:


Single head pressure injector with 100 syringe should be supplied.

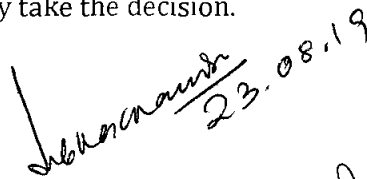
Full system UPS from reputed manufacturer having at least **30 minutes** backup with appropriate KVA to be supplied.


22. Standard and Safety:

Should be US FDA / CE approved, AERB approved.

Sl.no. 48 of term and conditions i.e "Downtime penalty clause during warranty and CAMC period", --- Purchase Section may take the decision.


23.8.19


23.08.19


23/8/19