

The following changes are made from previous specifications and terms & conditions.
Corrigendum for 64 Slice CT Scan machine :-

- a. The supply and installation of equipments for 64 slices CT scan machine is 120 days from date of issued supply order.
- b. The supply and installation of 64 Slices CT machine will be on Turnkey basis. The following items should be included on Turnkey basis.
 - i).Air Conditioner for whole system
 - ii).Lead Glass Window
 - iii).Lead Door
 - iv).LED view Box
 - v).Earthling wire for whole system
 - vi).Dehumidifier (2 nos.) & electronic pest control, 3 nos.

Sl.No. of the Technical Specification:

1. General:

- 3). The system should be US FDA/ CE approved, AERB approved.

2. Gantry:

- 1). The minimum scan time for a 360 degree should be less than as equal to 0.4 sec.

3. X-ray Generator and Tube:

- 4). X-ray tube should have focal spot size of less than or equal to 1 mm; smallest size should be 0.5 mm.

6). The X-ray tube Cooler Unit should be in-built in the Gantry. **The X-ray tube should have a cooling rate of 1300-1600 KHU per min.**


10. Work Station & Server:

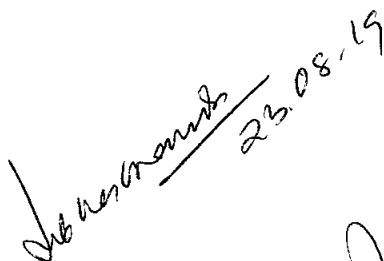
A multimodality client server architecture-based solution with minimum concurrent 16000 slice rendering capacity, with 32 GB RAM with storage of minimum 4 TB for CT, MRI & PET-CT visualization.


11. Misc.

3). Online UPS with maintenance free batteries capable of 30 minutes backup to run the entire system.

Sl.no.48 of terms and conditions i.e. "Downtime penalty clause during warranty and CAMC period", --- Purchase Section may take the decision.


23. 8. 19


23. 08. 19


23/8/19

The following changes are made from previous specifications and terms & conditions.
Corrigendum for 64 Slice CT Scan machine :-

- a. The supply and installation of equipments for 64 slices CT scan machine is 120 days from date of issued supply order.
- b. The supply and installation of 64 Slices CT machine will be on Turnkey basis. The following items should be included on Turnkey basis.
 - i).Air Conditioner for whole system
 - ii).Lead Glass Window
 - iii).Lead Door
 - iv).LED view Box
 - v).Earthling wire for whole system
 - vi).Dehumidifier (2 nos.) & electronic pest control, 3 nos.

Sl.No. of the Technical Specification:

1. **General:**

- 3). The system should be US FDA/ CE approved, AERB approved.

2. **Gantry:**

- 1). The minimum scan time for a 360 degree should be less than as equal to 0.4 sec.

3. **X-ray Generator and Tube:**

- 4). X-ray tube should have focal spot size of less than or equal to 1 mm; smallest size should be 0.5 mm.

6). The X-ray tube Cooler Unit should be in-built in the Gantry. **The X-ray tube should have a cooling rate of 1300-1600 KHU per min.**


10. **Work Station & Server:**

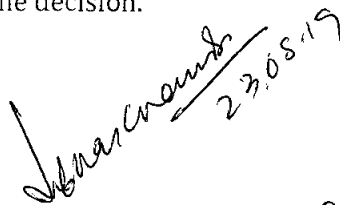
A multimodality client server architecture-based solution with minimum concurrent 16000 slice rendering capacity, with 32 GB RAM with storage of minimum 4 TB for CT, MRI & PET-CT visualization.


11. **Misc.**

3). Online UPS with maintenance free batteries capable of 30 minutes backup to run the entire system.

Sl.no.48 of terms and conditions i.e. "Downtime penalty clause during warranty and CAMC period", --- Purchase Section may take the decision.


23.8.19


23.08.19


23/8/19